

MULTI LIGAND CONTROL-TRI LEVEL LOT# MLAC1E2

PRODUCT CODE: ML-300 EXP: 2025-05-18

INTENDED USE

The Multi-ligand Controls are intended for use as an assayed quality control material to monitor the consistency of performance of laboratory test procedures associated with determination and monitoring of the clinical status. This product is a human-serum based, lyophilized control, stabilized with preservatives and can be used with all ELISA and CLIA methods.

SUMMARY AND EXPLANATION

The use of quality control material to assist in the assessment of precision in the clinical laboratory is an integral part of laboratory practices. Controls that contain varied levels of analytes are necessary to insure precision and accuracy in immunoassay systems.

REAGENTS

Monobind's Multi-ligand Controls are intended to be used in the exact manner as patient samples. The control is packaged as 6 vials of 3.0 ml, dried. The analyte activities are adjusted to concentrations in the low, middle and high range in order to monitor the efficacy of the procedure in use.

INSTRUCTIONS FOR USE

1) Bring the vials to room temperature before use.

2) Carefully unscrew and remove cap.3) Add three (3) ml of distilled or deionized water to each vial. Close the cap tightly and let the contents mix thoroughly for 30 minutes

4) Aliquot the materials in 0.5 ml aliquots in cryo vials and store at -20°C.

STORAGE, STABILITY AND DISPOSAL

This product will be stable until the expiration date when stored unopened at 2 to 8°C. Once the control is reconstituted, all analytes will be stable for 7 days when stored tightly capped at 2 to 8°C with the following exceptions: 1) C-Peptide should be assayed immediately after reconstitution, and 2) Folate and Insulin will be stable for 1 day. To avoid contamination, it is recommended labs aliquot required quantities into vials before each use.

After reconstituting, controls should be tightly capped and returned to refrigerator 2 to 8° C as soon as practical after usage. (Long term room temperature storage is not supported.) After reconstituting, controls should be tightly capped and frozen within 2-hours. Once thawed, do not refreeze the control; discard remaining material. It is recommended that customers aliquot control into separate containers before freezing to allow for usage on different days. Outdated material should be discarded as a biohazardous component.

STORAGE	STABILITY	TEMPERATURE
Lyophilized, Unopened	Three (3) years	< 8°C
Reconstituted, Opened	Seven (7) days	2 - 8°C
Reconstituted, Opened	Ninety (90) days	< -10°C

EXPECTED RANGE OF VALUES

The mean values printed in this insert were derived from replicate analyses and are specific for this lot of product. The tests listed were performed by Monobind QA using representative lots of this product, as well as those of Monobind's AccuBind® ELISA and AccuLite® CLIA reagents.


Individual laboratory means should fall within the corresponding acceptable range; however laboratory means may vary from the listed values during the life of this control. Therefore, each laboratory should establish its own means and acceptable ranges for the product used, using Monobind's assignment only as guide. A trend log should be maintained for batch to batch consistency of the test. Variations over time and between laboratories may be caused by a) differences in laboratory personnel, b) improper technique, c) instrumentation and reagents, d) improper dilutions from the stated manufacturer's procedure, and/ or e) modifications in the manufacturer's test procedure.


Refer to http://www.monobind.com/site/qc-documents.html for any updated insert information.

WARNING AND PRECAUTIONS

FOR IN VITRO DIAGNOSTIC USE

All products that contain human serum have been found to be non-reactive for HIV 1&2, HIV-Ag, HBsAg, HCV and RPR by FDA required tests. Since no known test can offer complete assurance that infectious agents are absent, all human serum products should be handled as potentially hazardous and capable of transmitting disease. Good laboratory procedures for handling blood products can be found in the Center for Disease Control / National Institute of Health, "Biosafety in Microbiological and Biomedical Laboratories," 2nd Edition, 1988, HHS Publication No. (CDC) 88-8395.

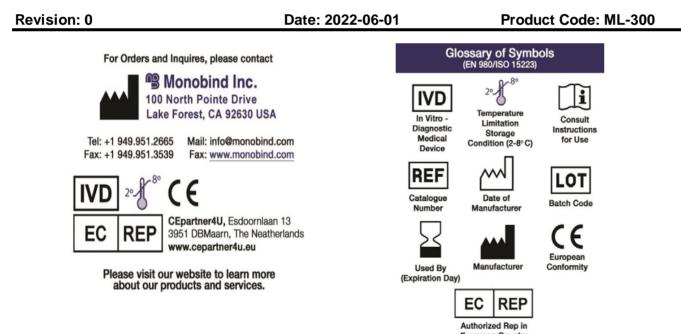



EXPECTED RANGE OF VALUES FOR MULTI-LIGAND CONTROL - TRI LEVEL

	А	В	С	
Analyte ergy	Range	Range	Range	Method
lgE in IU/mI emia	16.7 ± 5.51 17.5 ± 5.78	214.17 ± 70.68 230.2 ± 75.97	107 ± 35.31 106.8 ± 35.24	MB ACCULITE CLIA
Ferritin in ng/ml	39.8 ± 13.13 40.39 ± 13.33	76.7 ± 25.31 76.14 ± 25.13	419.33 ± 138.38 480.92 ± 158.70	MB ACCUBIND ELISA MB ACCULITE CLIA
Vitamin B12 in pg/ml	299.15 ± 98.72 330.76 ± 109.15	554.73 ± 183.06 560.33 ± 184.91	1041.71 ± 343.77 1106.86 ± 365.26	MB ACCUBIND ELISA MB ACCULITE CLIA
Folate in ng/ml emia Vast	2.27 ± 0.75 2.74 ± 0.90	6.14 ± 2.03 7.2 ± 2.38	9.09 ± 3.0 9.91 ± 3.27	MB ACCUBIND ELISA MB ACCULITE CLIA
(Vitamin B12) in pg/ml	230.02 ± 75.91 241.24 ± 79.61	517.05 ± 170.63 599.7 ± 197.9	1013.01 ± 334.29 860.18 ± 283.86	MB ACCUBIND ELISA MB ACCULITE CLIA
(Folate) in ng/ml	2.27 ± 0.75 2.74 ± 0.90	6.14 ± 2.03 7.2 ± 2.38	9.09 ± 3.0 9.91 ± 3.27	MB ACCULITE CLIA
Bone Metabolism Vit D Direct in ng/ml	21.05 ± 6.95	44.68 ± 14.75	98.05 ± 32.36	MB ACCUBIND ELISA
ncer Markers	22.05 ± 7.28	45.66 ± 15.07	115.94 ± 38.26	MB ACCURING FUSA
AFP in ng/ml	32 ± 10.56 28 ± 9.24 4.28 ± 1.41	115.3 ± 38.05 108 ± 35.64 15.24 ± 5.03	228.93 ± 75.55 207 ± 68.31 27.35 ± 9.03	MB ACCUBIND ELISA MB ACCULITE CLIA MB ACCUBIND ELISA
CEA in ng/ml CEA Next Generation in	4.8 ± 1.58 4.18 ± 1.38	17 ± 5.61 16.20 ± 5.35	30 ± 9.90 29.46 ± 9.72	MB ACCUBIND ELISA
ng/ml fPSA in ng/ml	4.09 ± 1.35 0.30 ± 0.10	16.26 ± 5.36 1.81 ± 0.60	30.32 ± 10.01 11.03 ± 3.64	MB ACCULITE CLIA MB ACCUBIND ELISA
tPSA-XS in ng/ml	0.43 ± 0.14 1.39 ± 0.46	1.98 ± 0.65 3.03 ± 1.00	13.23 ± 4.46 17.03 ± 5.62	MB ACCUBIND ELISA
tPSA in ng/ml	1.28 ± 0.42 2.97 ± 0.98 2.27 ± 0.75	3.01 ± 0.99 6.4 ± 2.11 5.47 ± 1.81	18.51± 6.11 36.3 ± 11.98 33.33 ± 11.0	MB ACCULITE CLIA MB ACCUBIND ELISA MB ACCULITE CLIA
ncer Markers Vast	4.45 ± 1.47	15.83 ± 5.22	26.17 ± 8.64	MB ACCUBIND ELISA
(CEA) in ng/ml (AFP) in ng/ml	4.26 ± 1.40 25.12 ± 8.29	18.29 ± 6.04 98.90 ± 32.64	27.98 ± 9.23 192.94 ± 63.67	MB ACCULITE CLIA MB ACCUBIND ELISA
(tPSA) in ng/ml	25.18 ± 9.40 1.44 ± 0.48	95.78 ± 31.61 4.23 ± 1.39	183.31 ± 60.49 23.86 ± 7.87	MB ACCULITE CLIA MB ACCUBIND ELISA
diac Markers	1.15 ± 0.38	3.90 ± 1.29	22.73 ± 7.50	MB ACCURING FUSA
Dig in ng/ml betes	0.45 ± 0.15 0.47 ± 0.15	1.55 ± 0.51 1.51 ± 0.50	3.10 ± 1.02 2.99 ± 0.99	MB ACCUBIND ELISA MB ACCULITE CLIA
C-Peptide in ng/ml	0.46 ± 0.15 0.39 ± 0.13	2.8 ± 0.92 2.97 ± 0.98	4.12 ± 1.36 4.36 ± 1.44	MB ACCUBIND ELISA MB ACCULITE CLIA
Insulin in µIU/mI	20.2 ± 6.67 18.7 ± 6.17	48.59 ± 16.03 51.7 ± 17.06	112.36 ± 37.08 114.6 ± 37.82	MB ACCUBIND ELISA MB ACCULITE CLIA
Rapid Insulin in µIU/mI tility	21.3 ± 7.03	48 ± 15.84	117 ± 38.61	MB ACCUBIND ELISA
FSH in mIU/mI	4.89 ± 1.61 4.41 ± 1.46 6.08 ± 2.01	24.53 ± 8.10 23.78 ± 7.85 31.48 ± 10.39	38.78 ± 12.80 37.86 ± 12.49 164.71 ± 54.35	MB ACCUBIND ELISA MB ACCULITE CLIA MB ACCUBIND ELISA
hCG in mIU/mI	4.5 ± 1.49 4.40 ± 1.45	41.2 ± 13.60 24.95 ± 8.23	217.4 ± 71.74 158.90 ± 52.44	MB ACCUBIND ELISA MB ACCUBIND ELISA MB ACCUBIND ELISA
hCG-XR in mIU/mI	3.89 ± 1.28 4.43 ± 1.46	23.99 ± 7.92 23.60 ± 7.79	147.32 ± 48.62 51.47 ± 16.99	MB ACCUBIND ELISA
PRL in ng/ml	4.18 ± 1.38 5.48 ± 1.81	24.05 ± 7.94 21.2 ± 7	51.63 ± 17.04 73.16 ± 24.14	MB ACCULITE CLIA MB ACCUBIND ELISA
PRL-seq in ng/ml	4.4 ± 1.45 3.94 ± 1.49	18.5 ± 6.11 13.17 ± 4.35	66.6 ± 21.98 33.68 ± 11.11	MB ACCULITE CLIA MB ACCUBIND ELISA
Rapid HCG in mIU/mI	3.91 ± 1.29 6.05 ± 2.00	12.79 ± 4.22 32.04 ± 10.57	29.35 ± 9.68 166.16 ± 54.83	MB ACCUBIND ELISA
(FSH) in mIU/mI	27.19 ± 8.97 25.18 ± 8.31	115.80 ± 38.21 110.00 ± 36.30	212.27 ± 70.05 216.40 ± 71.41	MB ACCUBIND ELISA MB ACCULITE CLIA
(LH) in mIU/mI	1.03 ± 0.34 1.19 ± 0.39	2.90 ± 0.96 2.58 ± 0.85	6.11 ± 2.01 5.81 ± 1.92	MB ACCULITE CLIA
(hCG) in mIU/mI	4.05 ± 1.34 4.74 ± 1.56	27.80 ± 9.17 25.43 ± 8.39	139.0 ± 45.87 141.98 ± 46.85	MB ACCUBIND ELISA MB ACCULITE CLIA
ole Screen VAST (AFP) in ng/ml	27.19 ± 8.97	115.80 ± 38.21	212.27 ± 70.05	MB ACCUBIND ELISA
(uE3) in ng/ml	25.18 ± 8.31 1.03 ± 0.34 1.19 ± 0.39	110.00 ± 36.30 2.90 ± 0.96 2.58 ± 0.85	216.40 ± 71.41 6.11 ± 2.01 5.81 ± 1.92	MB ACCULITE CLIA MB ACCUBIND ELISA MB ACCULITE CLIA
(hCG) in mIU/mI	4.05 ± 1.34 4.74 ± 1.56	27.80 ± 9.17 25.43 ± 8.39	139.0 ± 45.87 141.98 ± 46.85	MB ACCULITE CLIA
hGH in µIU//mI	7.23 ± 2.39	26.1± 8.61	63.76 ± 21.04	MB ACCUBIND ELISA
roids	7 ± 2.31	28.2 ± 9.31	60.5 ± 19.97	MB ACCULITE CLIA
Cortisol in µg/dl	2.79 ± 0.92 2.83 ± 0.94 0.34 ± 0.11	15.30 ± 5.05 13.64 ± 4.50 1.35 ± 0.45	29.40 ± 9.70 28.56 ± 9.42 4.38 ± 1.45	MB ACCUBIND ELISA MB ACCULITE CLIA MB ACCUBIND ELISA
DHEA-S in µg/ml	0.44 ± 0.15 0.73 ± 0.33	1.6 ± 0.53 4.03 ± 1.33	4.5 ± 1.49 9.09 ± 3.0	MB ACCULITE CLIA MB ACCUBIND ELISA
DHEA in ng/ml E2 in pg/ml	0.72 ± 0.24 30.26 ± 9.98	4.58 ± 1.51 169.49 ± 55.93	9.51 ± 3.14 329.01 ± 108.57	MB ACCULITE CLIA MB ACCUBIND ELISA
Progesterone in ng/ml	28.75 ± 9.49 1.1± 0.36	171.0 ± 56.43 8.44 ± 2.79	348.85 ± 115.12 24.59 ± 8.11	MB ACCULITE CLIA MB ACCUBIND ELISA
17-OHP in ng/ml	1.4 ± 0.46 0.50 ± 0.17	10 ± 3.30 2.09 ± 0.69	26.5 ± 8.75 5.33 ± 1.87	MB ACCUBIND ELISA
17-OHP-SI in ng/ml	0.55 ± 0.18 0.35 ± 0.12 0.31 ± 0.10	2.14 ± 0.71 1.13 ± 0.37 1.33 ± 0.44	5.34 ± 1.76 3.15 ± 1.04 3.66 ± 1.21	MB ACCULITE CLIA MB ACCUBIND ELISA MB ACCULITE CLIA
Testosterone in ng/ml	0.29 ± 0.09 0.37 ± 0.12	1.21 ± 0.40 1.28 ± 0.42	6.62 ± 2.18 7.34 ± 2.42	MB ACCUBIND ELISA MB ACCULITE CLIA
uE3 in ng/ml	1.13 ± 0.42 1.15 ± 0.38	2.40 ± 0.79 2.51 ± 0.83	6.27 ± 2.07 5.78 ± 1.91	MB ACCUBIND ELISA MB ACCULITE CLIA
E1 in ng/ml	42.69 ± 14.09 43.68 ± 14.41	191.59 ± 63.22 213.38 ± 70.42	508.55 ± 167.82 488.08 ± 161.06	MB ACCULITE CLIA
ANST in ng/ml Aldosterone in ng/ml	0.32 ± 0.11 85.84 ± 28.33	0.86 ± 0.28 342.19 ± 112.92	7.1 ± 2.34 1011.35 ± 333.75	MB ACCUBIND ELISA MB ACCUBIND ELISA
Free Testosterone (0-60pg/ml calibration)	86.9 ± 28.68 0.93 ± 0.31 0.97 ± 0.32	401.2 ± 132.40 2.63 ± 0.87 2.66 ± 0.88	1112.74 ± 367.20 20.29 ± 6.70 27.24 ± 8.99	MB ACCULITE CLIA MB ACCUBIND ELISA MB ACCULITE CLIA
roid	0.51 ± 0.17	1.35 ± 0.45	3.43 ± 1.13	MB ACCUBIND ELISA
T3 in ng/ml T4 in μg/dl	0.59 ± 0.24 2.82 ± 0.93	1.43 ± 0.47 6.54 ± 2.16	3.27 ± 1.08 16.48 ± 5.44	MB ACCULITE CLIA MB ACCUBIND ELISA
TSH in µIU/mI	2.75 ± 0.91 0.40 ± 0.13	6.60 ± 2.18 $4.00 + 1.32$	15.33 ± 5.06 20.22 ± 6.67	MB ACCULITE CLIA MB ACCUBIND ELISA
fT3 in pg/ml	0.42 ± 0.14 2.01 ± 0.66	4.00 ± 1.32 4.11 ± 1.36	21.39 ± 7.06 8.53 ± 2.81	MB ACCUBIND ELISA
fT4 in ng/dl	2.24 ± 0.74 0.52 ± 0.17 0.54 ± 0.18	4.12 ± 1.36 1.28 ± 0.42 1.19 ± 0.39	7.98 ± 2.63 4.06 ± 1.34 3.83 ± 1.26	MB ACCULITE CLIA MB ACCUBIND ELISA MB ACCULITE CLIA
T3-Uptake in %U	32.35 ± 1.86 31.55 ± 2.42	30.65 ± 1.86 30.88 ± 2.34	46.15 ± 1.85 46.55 ± 2.70	MB ACCULITE CLIA MB ACCULITE CLIA
Rapid TSH in µIU/ml	0.59 ± 0.20 0.31 ± 0.12	4.17 ± 1.37 4.05 ± 1.34	19.63 ± 648 21.0 ± 6.93	MB ACCUBIND ELISA MB ACCULITE CLIA
TSH-RC in µIU/mI yroid VAST	0.56 ± 0.18	4.61 ± 1.52	21.88 ± 7.22	MB ACCUBIND ELISA
(TSH) in μlU/ml	0.37 ± 0.12 0.31 ± 0.10	4.18 ± 1.38 4.32 ± 1.43	22.95 ± 7.57 24.24 ± 8.00	MB ACCULITE CLIA
Strep T3 in ng/ml	0.51 ± 0.17 0.47 ± 0.16 3.27 ± 1.08	1.46 ± 0.48 1.32 ± 0.43 8.54 ± 2.82	3.15 ± 1.04 3.14 ± 1.04 17.19 ± 5.67	MB ACCUBIND ELISA MB ACCULITE CLIA MB ACCUBIND ELISA
Strep T4 in µg/dl e Thyroid VAST	3.27 ± 1.08 2.98 ± 0.98	8.54 ± 2.82 8.26 ± 2.73	17.19 ± 5.67 16.29 ± 5.37	MB ACCULITE CLIA
(TSH) in μlU/ml	0.46 ± 0.15 0.53 ± 0.17	4.64 ± 1.53 4.87 ± 1.61	23.78 ± 7.85 22.56 ± 7.44	MB ACCUBIND ELISA MB ACCULITE CLIA
Strept fT3 in pg/ml	1.81 ± 0.60 1.79 ± 0.59	3.42 ± 1.13 3.87 ± 1.28	9.78 ± 4.20 8.64 ± 2.85	MB ACCUBIND ELISA MB ACCULITE CLIA
	0.91 ± 0.30	3.87 ± 1.28 1.25 ± 0.41	5.22 ± 1.72	MB ACCUBIND ELISA